



Clinical Review


Dr. Joseph Amos



Nevro Spinal Cord Stimulator Trial Outcomes


Responder Rate = 97%

■ Responded ■ Not responded

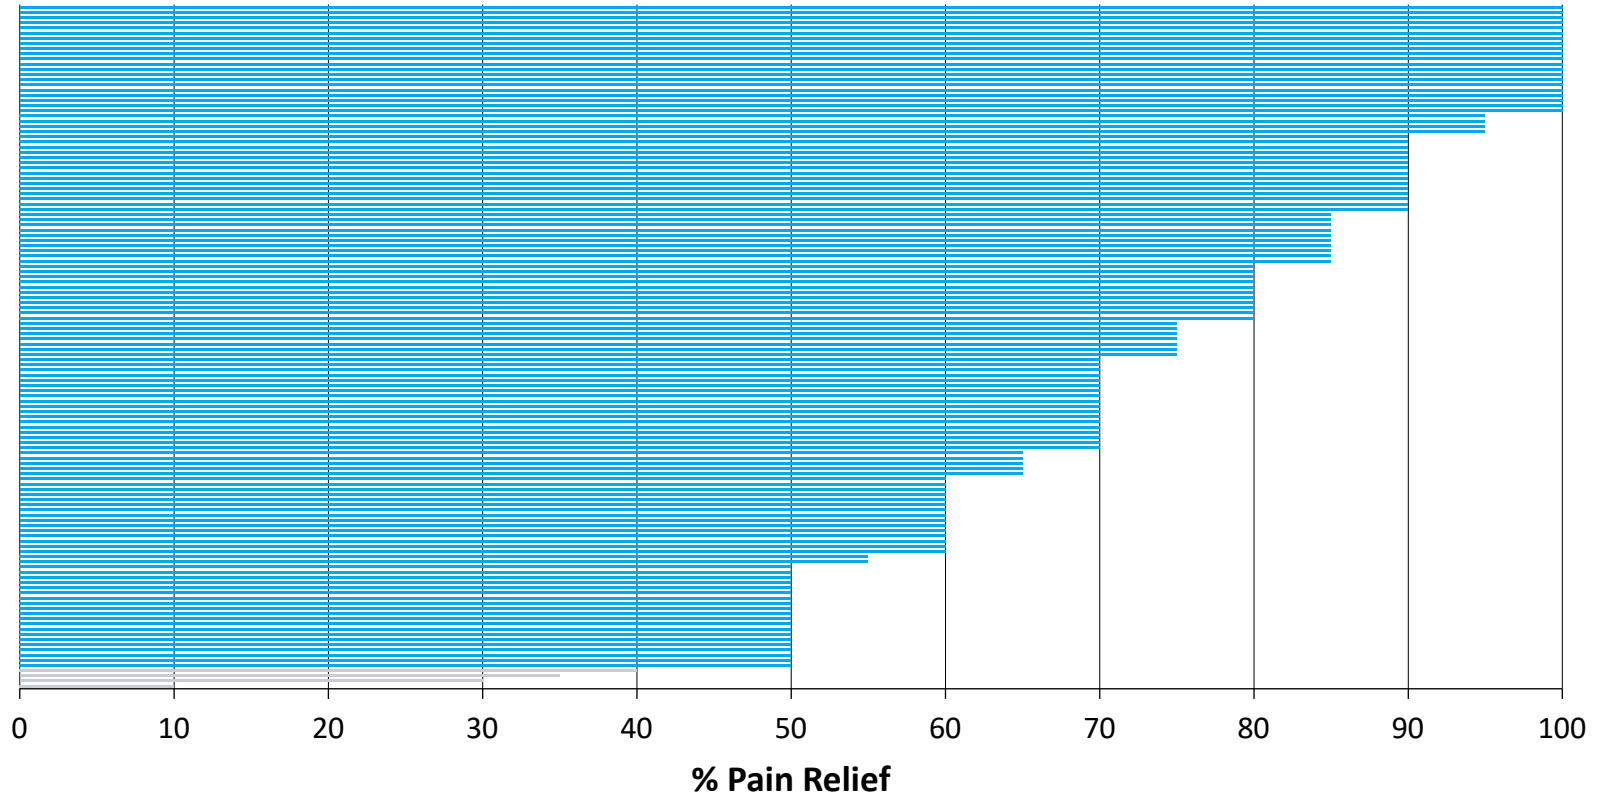


Patient Preferred Waveform Analysis

Programmed Waveforms

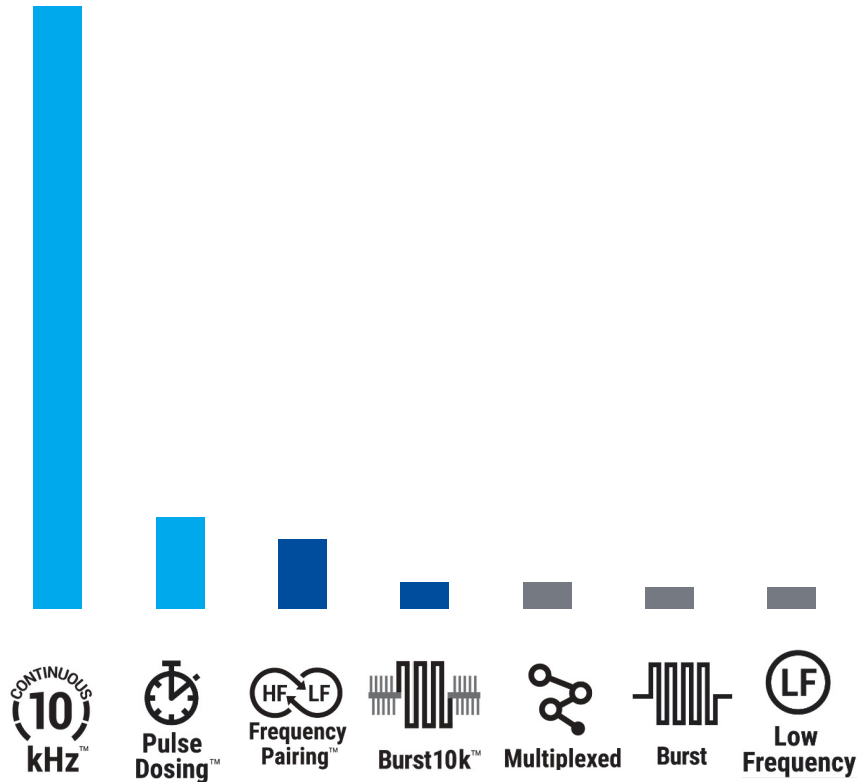


Current Waveforms

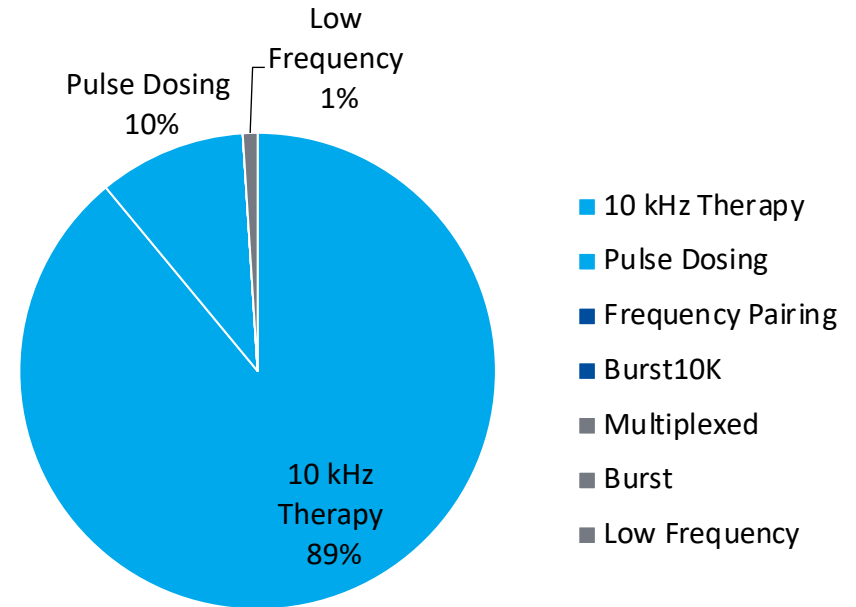


Change in Quality of Life Measures

Change in Medication Use

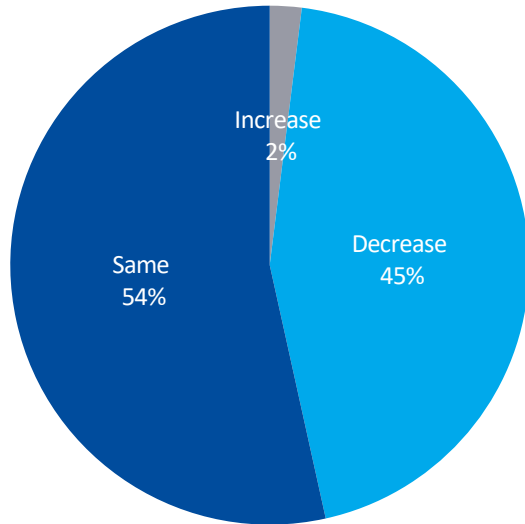

Improvement in Sleep

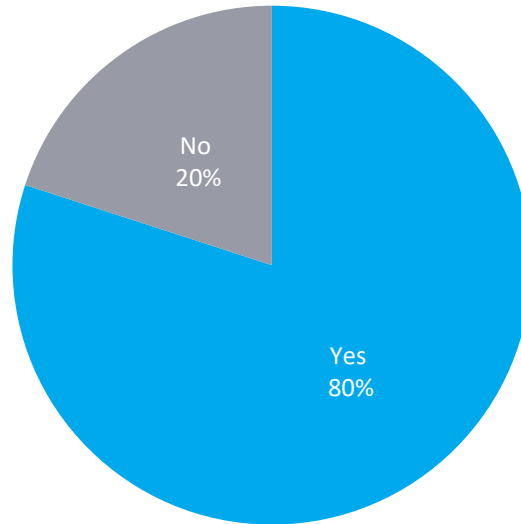

Improvement in Function

